



PRECAUTIONS:

- Please be cautious with your cultured embryos, considering that during the measurement procedure the composition of the gas in the chamber may be affected.
- Read the manuals for the incubator and LEO 2.0 for usage and safety details.



Evaluate the need for chamber cleaning and disinfection after working on the incubator.



As good practice, it is recommended to have LEO 2.0 charged before use, and not to charge it during use.



Always read the manual of the devices.





If LEO 2.0 shows a message that it's warming up, it is advised to complete the warm up period before using.


STEP 1 Set **EMBRYOSCOPE** to **Validation Mode**, and if you prefer **37.0°C**.




STEP 2 Place **LEO 2.0's** temperature probe (T1-MODULE) inside a culture dish well, so that the tip of the sensor touches the bottom of the dish.

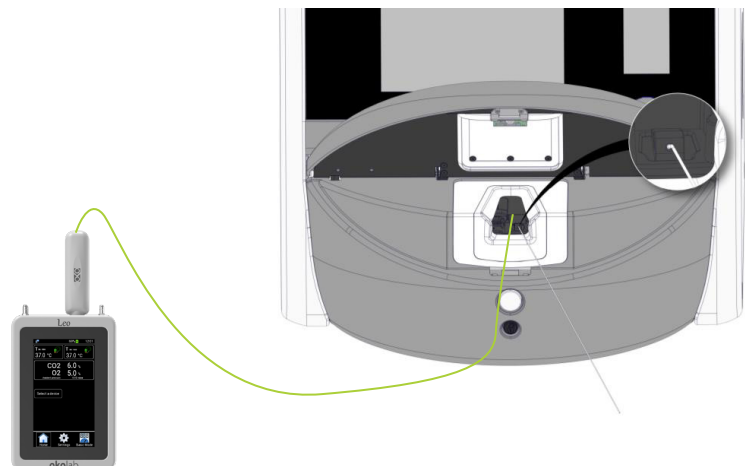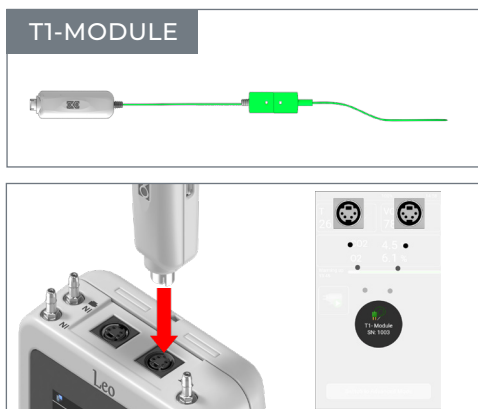


STEP 3 Fix the cable of **LEO 2.0's** probe so that it will not move from its position.

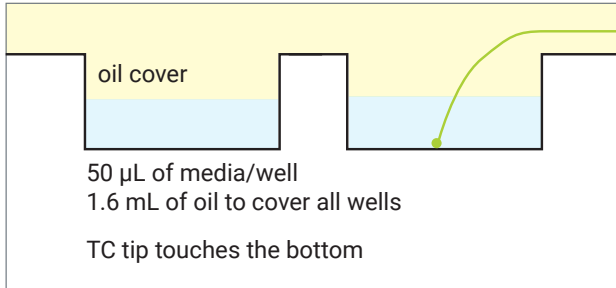

STEP 4 Close the lids of **EMBRYOSCOPE**.

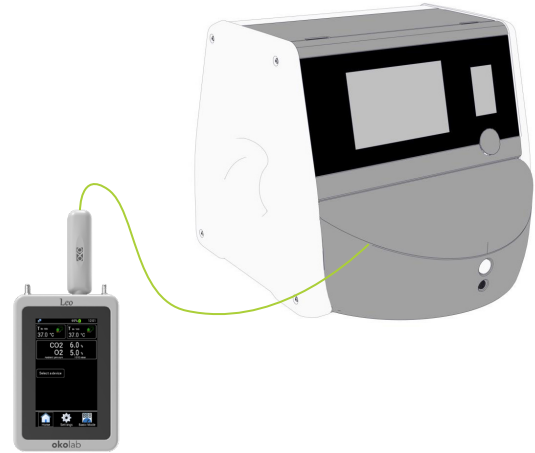

STEP 5 Give enough time for **EMBRYOSCOPE** and the media to thermally stabilize.

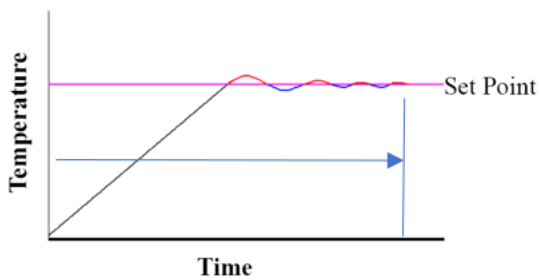

If the temperature on **LEO 2.0's** display is stable for a period of 10 minutes, proceed to **Step 6**.

STEP 6 Take the reading from **LEO 2.0**.



Read LEO 2.0 User Manual for details.

